



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:  
**09.08.2000 Bulletin 2000/32**

(51) Int Cl.7: **A61B 17/04**

(21) Application number: **00890034.2**

(22) Date of filing: **03.02.2000**

(84) Designated Contracting States:  
**AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU**  
**MC NL PT SE**  
Designated Extension States:  
**AL LT LV MK RO SI**

(72) Inventors:  
• **Grafton, Donald R.**  
**Naples, Florida 34104 (US)**  
• **Brunsvold, Mark**  
**Naples, Florida 34102 (US)**

(30) Priority: **04.02.1999 US 118788 P**  
**21.12.1999 US 469177**


(74) Representative: **Kopecky, Helmut, Dipl.-Ing.**  
**Kopecky & Schwarz Patentanwälte et al**  
**Wipplingerstrasse 32/22**  
**1010 Wien (AT)**

(71) Applicant: **Arthrex, Inc.**  
**Naples, FL 34104 (US)**

(54) **Headed bioabsorbable tissue anchor**

(57) A headed bioabsorbable tissue anchor (2) has a continuous thread (6) spiraling around a tapering central core (4). At the distal end, the headed bioabsorbable tissue anchor terminates in a flat point (16). At the proximal end, the bioabsorbable tissue anchor has a flat,

disk-shaped head (10) for engaging tissue, and slots (12) formed in the head for engaging a driver (30). The headed bioabsorbable tissue anchor has a large thread surface per turn of thread. As the anchor is turned into bone for engaging cancellous bone, the disk-shaped head (10) engages and anchors the tissue to the bone.

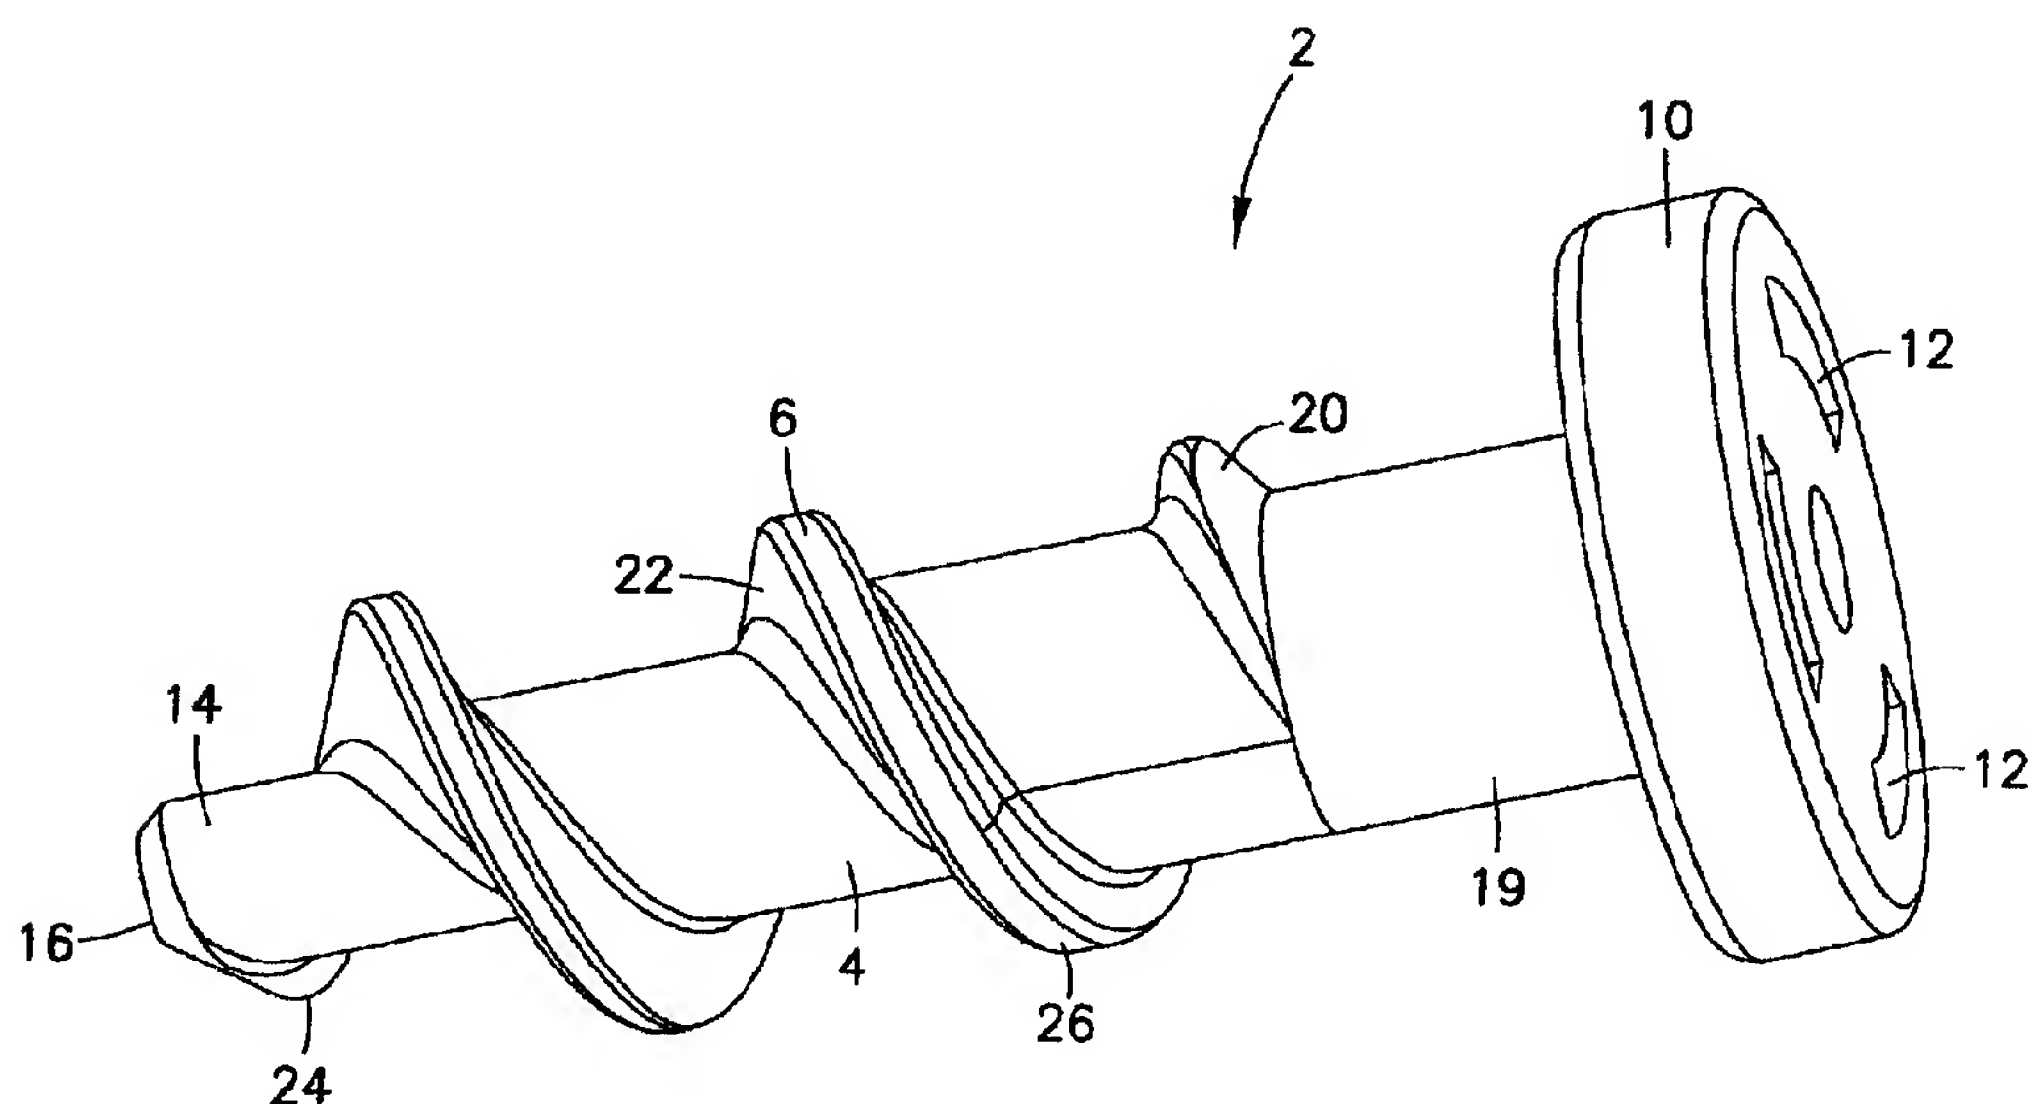

**Fig. 3**

## Description

### BACKGROUND OF THE INVENTION

#### 1. Field of the Invention:

**[0001]** The present invention relates to an apparatus and method for fixation of soft tissue to bone. More specifically, the present invention relates to sutureless arthroscopic apparatus and methods for anchoring soft tissue to bone using a headed bio-absorbable tissue anchor.

#### 2. Description of the Related Art:

**[0002]** When soft tissue tears away from bone, reattachment becomes necessary. Various fixation devices, including sutures, screws, staples, wedges, and plugs have been used in the past to secure soft tissue to bone. More recently, various types of threaded suture anchors have been developed.

**[0003]** The known suture anchors generally require that the surgeon tie knots in the suture to secure tissue to the bone. Tying surgical knots is tedious and time-consuming. It would be preferable to be able to secure the soft tissue to the bone in one step without having to tie knots.

**[0004]** Accordingly, a need exists for a bioabsorbable anchor for soft tissue fixation that can be installed to secure tissue easily and effectively without sutures. A need also exists for a soft tissue fixation device that displaces a minimum amount of bone upon insertion. In addition, a need exists for a tissue fixation device having exceptional pull-out strength, especially in soft bone.

### SUMMARY OF THE INVENTION

**[0005]** The present invention overcomes disadvantages of the prior art, such as those noted above, by providing a headed bioabsorbable tissue anchor having a thread spiraling helically around a central body, in which the head of the anchor engages the soft tissue for fixation to bone.

**[0006]** The headed bioabsorbable tissue anchor of the present invention has a cannulated, threaded central body. A flat, disk-shaped head is provided on the proximal end of the anchor. The disk-shaped head engages soft tissue for fixation as the anchor is installed through soft tissue and into bone.

**[0007]** The central body of the anchor tapers toward the distal end. The distal tip preferably is flat to avoid tip breakage, as could occur with a pointed tip.

**[0008]** The anchor is formed of a bioabsorbable PLA copolymer, preferably poly (L/D-lactide) acid.

**[0009]** Surgical installation is achieved using a driver that engages the disk-shaped head for installing the threaded anchor by turning into the bone. The anchor has at least one opening for engagement with the end

of a driver.

**[0010]** The outer circumferential dimension of the disk-shaped head advantageously is substantially larger than the circumference of the central body. Accordingly, the enlarged head engages tissue and holds it in place against the bone into which the tissue anchor has been installed.

**[0011]** Advantageously, the threads of the headed bioabsorbable tissue anchor of the present invention have a cancellous thread design that provides an increased percentage of thread surface area for each turn of the anchor, as compared with known anchors, thus providing increased pull-out strength, and a decreased tendency for back-out.

**[0012]** In addition to increased pull-out strength, the one piece sutureless design of the implant advantageously eliminates suture management issues, and simplifies the arthroscopic surgical technique. Further, revisions are simplified, and the biocompatible PLA copolymer material will not interfere with MRI or CT scans. The wide, low profile head provides a broad area of tissue to bone contact without impingement on other tissues. Also, the cannulated design allows the use of a guide wire to ensure accurate implant placement. The implant also can be used in open procedures.

**[0013]** Other features and advantages of the present invention will become apparent from the following description of the invention, which refers to the accompanying drawings.

### BRIEF DESCRIPTION OF THE DRAWINGS

**[0014]** Fig. 1 is a side elevation of a headed bioabsorbable tissue anchor according to the present invention.

**[0015]** Fig. 2 is a cut-away side elevation of the headed bioabsorbable tissue anchor of Fig. 1.

**[0016]** Fig. 3 is a perspective view of the headed bioabsorbable tissue anchor of Fig. 1.

**[0017]** Fig. 4 is an elevation of a driver according to the present invention.

**[0018]** Fig. 5 is an elevation of a tap according to the present invention.

**[0019]** Fig. 6 is an elevation of a 1.0 mm guide wire used for installation of the headed anchor according to the present invention.

**[0020]** Fig. 7 is an elevation of a spear used to facilitate insertion of the guide wire according to the present invention.

**[0021]** Fig. 8 is a perspective view of the tissue anchor of Fig. 1 assembled onto the driver of Fig. 4 and disposed over the guide wire of Fig. 6.

**[0022]** Fig. 9 is a schematic illustration of the tissue anchor of Fig. 1 installed through tissue and into bone.

## DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

**[0023]** Referring to Figs. 1-3, the headed bioabsorbable tissue anchor **2** of the present invention includes a body **4** provided in the shape of a cannulated, tapered cylinder. A continuous thread **6** wraps around body **4** in a clockwise direction, as shown. The thread preferably has an outer diameter of 5.0 mm. The outer diameter of the thread remains substantially constant, while the inner diameter of the thread decreases distally, following the taper of the body **4**. Accordingly, the surface area of the thread increases distally. The central core of body **4** preferably is circular in cross-section, and tapers from a maximum diameter near the proximal end to a minimum diameter toward the distal end.

**[0024]** Headed bioabsorbable tissue anchor **2** is provided at the proximal end of body **4** with a head **10**. The anchor is provided with at least one opening for engaging a driver. Although many different drive coupling arrangements are possible, in the preferred embodiment of the invention, equally spaced arcuate slots **12** are formed in the disk-shaped head to engage the driver described more fully below. The driver is used for delivery and installation of the anchor. Slots **12** formed in the head of the anchor preferably taper to enhance retention of the anchor on the distal end of the driver. The head **10** is 8.0 mm in diameter to provide a broad area of tissue-to-bone contact, and has a smooth, low 1.5 mm thick profile to minimize trauma to surrounding tissue.

**[0025]** At the distal tip **14**, the anchor terminates in a flat end **16**. The flat end is less likely than a pointed tip to break off and become a loose body within the patient. Cannula **18** is provided centrally. Preferably, the cannula has a circular cross-section; however, the cannula could be shaped to engage a driver for installation of the anchor by turning. Accordingly, the cannula could be hexagonal or provided with ridges, for example.

**[0026]** The head **10** preferably is separated from the thread **6** by a smooth section **19** that passes through and accommodates the tissue atraumatically upon insertion of the anchor into bone, as described more fully below.

**[0027]** The anchor preferably is formed of a bioabsorbable, biocompatible material. Preferably, the anchor material is a PLA copolymer, most preferably poly (L/D-lactide) acid (PLDLA) having a high inherent viscosity.

**[0028]** Anchor thread **6** has a proximal face **20**, a distal face **22** and an edge. Near distal tip **14**, the edge is formed at an acute angle to the proximal face so as to provide a V-shaped edge **24** that provides a better purchase on the bone as the anchor is advanced by turning during installation. Proceeding proximally along the anchor thread, the thread widens toward a U-shape and the edge becomes substantially parallel with the central axis of the anchor to provide a flat edge **26**. The thickness of the thread **6** increases, preferably continuously,

from the distal end to the proximal end, as the profile of the edge changes from the sharp V edge **24** to the increasingly wider flat edge **26**. The overall configuration provides a spiral wedge that enhances fixation.

**[0029]** Preferably, between two and three flights or turns of thread **6** are provided along body **4**, between the proximal end and the distal tip. Adjacent sections of each flight are separated by a gap that is determined by the number of turns per inch of the thread.

**[0030]** Increased surface area of the thread also is achieved in part by providing an increased ratio of the outer diameter of the thread to the inner diameter of the thread along at least a portion of the anchor. Preferably, the ratio is between 2.25 and 2.75. Most preferably, the ratio of the outer diameter to the inner diameter is at least 2.5 along at least a portion of the thread.

**[0031]** In addition, the headed bioabsorbable tissue anchor has a higher thread pitch than prior art screws, thus increasing the area of thread for each turn of the screw, which leads also to greater pull-out strength and faster installation. Significantly, due to the increased pitch, fewer turns are required to advance the headed bioabsorbable tissue anchor into position during installation of the device. Accordingly, the headed bioabsorbable tissue anchor is easy to install, and displaces less tissue material upon insertion than known anchors.

**[0032]** The pull-out strength and minimal tissue damage are enhanced by the relatively compressed cross-sectional aspect of the thread, particularly in relation to the broad axial faces of the threads. Further, in contrast to the tapered central axis, the threads maintain a substantially fixed outer diameter along their length.

**[0033]** Increased back-out resistance can be enhanced further by surface features, such as indentations or radial ridges, on the top and/or bottom faces of the screw threads. The surface features augment the engagement between the thread surfaces and the surrounding tissue once the headed bioabsorbable corkscrew is installed.

**[0034]** Fig. 4 illustrates a preferred headed bioabsorbable tissue anchor driver **30** according to the present invention. The driver **30** has a cannulated shaft **32** attached to a cannulated handle **34**. At the distal end of shaft **32** a head **36** includes three arcuate projections **38** which engage the tapered, arcuate slots **12** formed in the head of the screw **2**.

**[0035]** Fig. 5 illustrates a cannulated tap **40** according to the present invention. The tap **40** includes a shaft **42** and a handle **44**. Tap **40** has a tap head **46** provided on the distal end of the instrument. The tap head **46** has a trocar tip **48** and thread **50** for entering and tapping bone prior to insertion of the bioabsorbable corkscrew **2**. A depth stop **52** engages the tissue to indicate an appropriate depth of insertion, as described below.

**[0036]** The configuration of the distal end of tap **50** is substantially similar to the configuration of the threaded portion of the anchor, described above. Advantageously, the outer diameter of the thread **50** on the tap is small-

er than the outer diameter of the thread **6** on the anchor, typically by about 5%. Accordingly, the anchor thread **6** compresses bone tissue as it is installed by turning into the thread formed by the smaller tap thread **50**. The forced fit enhances fixation strength. In a preferred embodiment, for example, the outer diameter of the tap thread is 5.0 mm, and the outer diameter of the tap thread is 4.78 mm.

**[0037]** The present invention also provides an assembly of the headed bioabsorbable tissue anchor and the driver for installing the anchor. Referring to Fig. 8, the tissue anchor **2** is shown engaged on the end of driver **30**. The assembly has been placed over a guide wire **60**, as described below with respect to a preferred method of installation.

**[0038]** Indications for the headed bioabsorbable tissue anchor of the present invention include rotator cuff repair (full or partial tears), Bankart repair, SLAP lesion repair, biceps tenodesis, acromio-clavicular separation repair, deltoid repair, and capsular shift or capsulolabral reconstruction in the shoulder; lateral stabilization, medial stabilization, achilles tendon repair, hallux valgus reconstruction, midfoot reconstructions, and metatarsal ligament repair in the foot/ankle; medial collateral ligament repair, lateral collateral ligament, patellar tendon repair, posterior oblique ligament repair, and iliotibial band tenodesis in the knee; scapholunate ligament reconstruction, ulnar collateral ligament reconstruction, and radial collateral ligament reconstruction in the hand/wrist; and biceps tendon reattachment, tennis elbow repair, and ulnar or radial collateral ligament reconstruction in the elbow.

**[0039]** Referring to Figs. 6-9, an illustrative, generalized method of securing soft tissue to bone using the headed bioabsorbable tissue anchor of the present invention received over a guide wire **60** is described as follows:

1. Prepare a bone bed site **62** by debriding the site with a high-speed bur or rasp.
2. Move the tissue **64** into the proper position apposing the prepared bone site **62**.
3. Install a 1.0 mm guide wire **60** by advancing the guide wire through the tissue **64** and into the prepared bone bed **62** at an appropriate angle. See Fig. 6. Installation of the guide wire can be facilitated by inserting the guide wire through a cannulated spear **70** (Fig. 7) that has been used to pierce the tissue and firmly engage the bone surface with its pointed tip.
4. Place the cannulated tap **40** over the exposed guide wire **60** and advance by turning through the tissue and into the bone. The tap is advanced until the depth stop collar **52** depresses the tissue. Remove the tap by turning in the direction opposite to installation, while holding the guide wire in place.
5. Place the headed tissue anchor over the guide wire. Place the cannulated driver over the guide

wire to engage the head of the anchor. See Fig. 8.  
6. Advance the anchor by turning clockwise through the tissue and into the bone until the head of the implant depresses the tissue. See Fig. 9.

7. Repeat the installation steps, inserting additional anchors at other tissue locations for further fixation, as needed.

8. Remove the guide wire.

**[0040]** Accordingly, in a preferred method of rotator cuff repair, for example, the rotator cuff is retracted laterally and the spear **70** is inserted through the tendon. The guide wire **60** is advanced by turning into the debrided portion of the humerus. The tap, aligned over the guide wire, is turned through the tendon and into bone until the collar slightly depresses the tendon. During tap removal, a guide wire pusher (not shown) inserted into the back of the tap is used to keep the guide wire in place. The cannulated anchor is placed over the guide wire and atraumatically turned using a driver through the tendon into bone until the cuff is firmly apposed against bone. The guide wire is removed.

**[0041]** The broad apposition and compression of soft tissue to bone provided by the present invention speeds healing and provides a stronger soft tissue fixation, compared to sutures. Concurrently, the smooth upper surface of the anchor head **10** allows atraumatic articulation of the repaired joint. The cancellous thread provides enhanced thread purchase through the outer cortical bone layer. The anchor of the present invention withstands up to 90 pounds of pull-out force prior to failure. In addition, the PLA copolymer (PLDLA) material has a high inherent viscosity, and in degradation studies the anchor retains 90% of its fixation strength after 12 weeks.

**[0042]** Although the present invention has been described in relation to particular embodiments thereof, many other variations and modifications and other uses will become apparent to those skilled in the art. Therefore, the present invention is to be limited not by the specific disclosure herein, but only by the appended claims.

## Claims

1. A headed bioabsorbable tissue anchor, comprising:
  - a fully cannulated body formed of a bioabsorbable material, the body having a distal end and a proximal end;
  - a continuous thread disposed in a spiral around the body and having an outer diameter;
  - a head disposed on the proximal end of the body for engaging tissue, the head having an outer diameter greater than the outer diameter of the thread; and
  - at least one opening formed in the anchor for engaging a driver for turning the anchor.

2. The tissue anchor of claim 1, wherein the at least one opening formed in the anchor for engaging a driver for turning the anchor extends completely through the head of the anchor. 5
3. The tissue anchor of claim 2, wherein the at least one opening formed in the head comprises three arcuate slots for engaging the driver.
4. The tissue anchor of claim 1, wherein the ratio of the outer diameter of the thread to an inner diameter of the thread is about 2.5. 10
5. The tissue anchor of claim 1, wherein the thread increases in thickness from the proximal end to the distal end. 15
6. The tissue anchor of claim 1, wherein the outer diameter of the thread is substantially constant from the proximal end to the distal end. 20
7. The tissue anchor of claim 1, wherein the body tapers from the proximal end to the distal end.
8. The tissue anchor of claim 1, further comprising a flat tip disposed on the distal end of the body. 25
9. The tissue anchor of claim 1, wherein the tissue anchor is formed of a PLA co-polymer comprising poly (L/D-lactide) acid. 30
10. A headed bioabsorbable tissue anchor and driver assembly for driving a headed bioabsorbable tissue anchor into bone, the assembly comprising: 35
  - a driver having a distal end and a proximal end, the distal end having a plurality of projections; and
  - a headed bioabsorbable tissue anchor inserted on the distal end of the driver, the head of the corkscrew being disk-shaped and having slots engaging the plurality of projections on the driver. 40

45

50

55



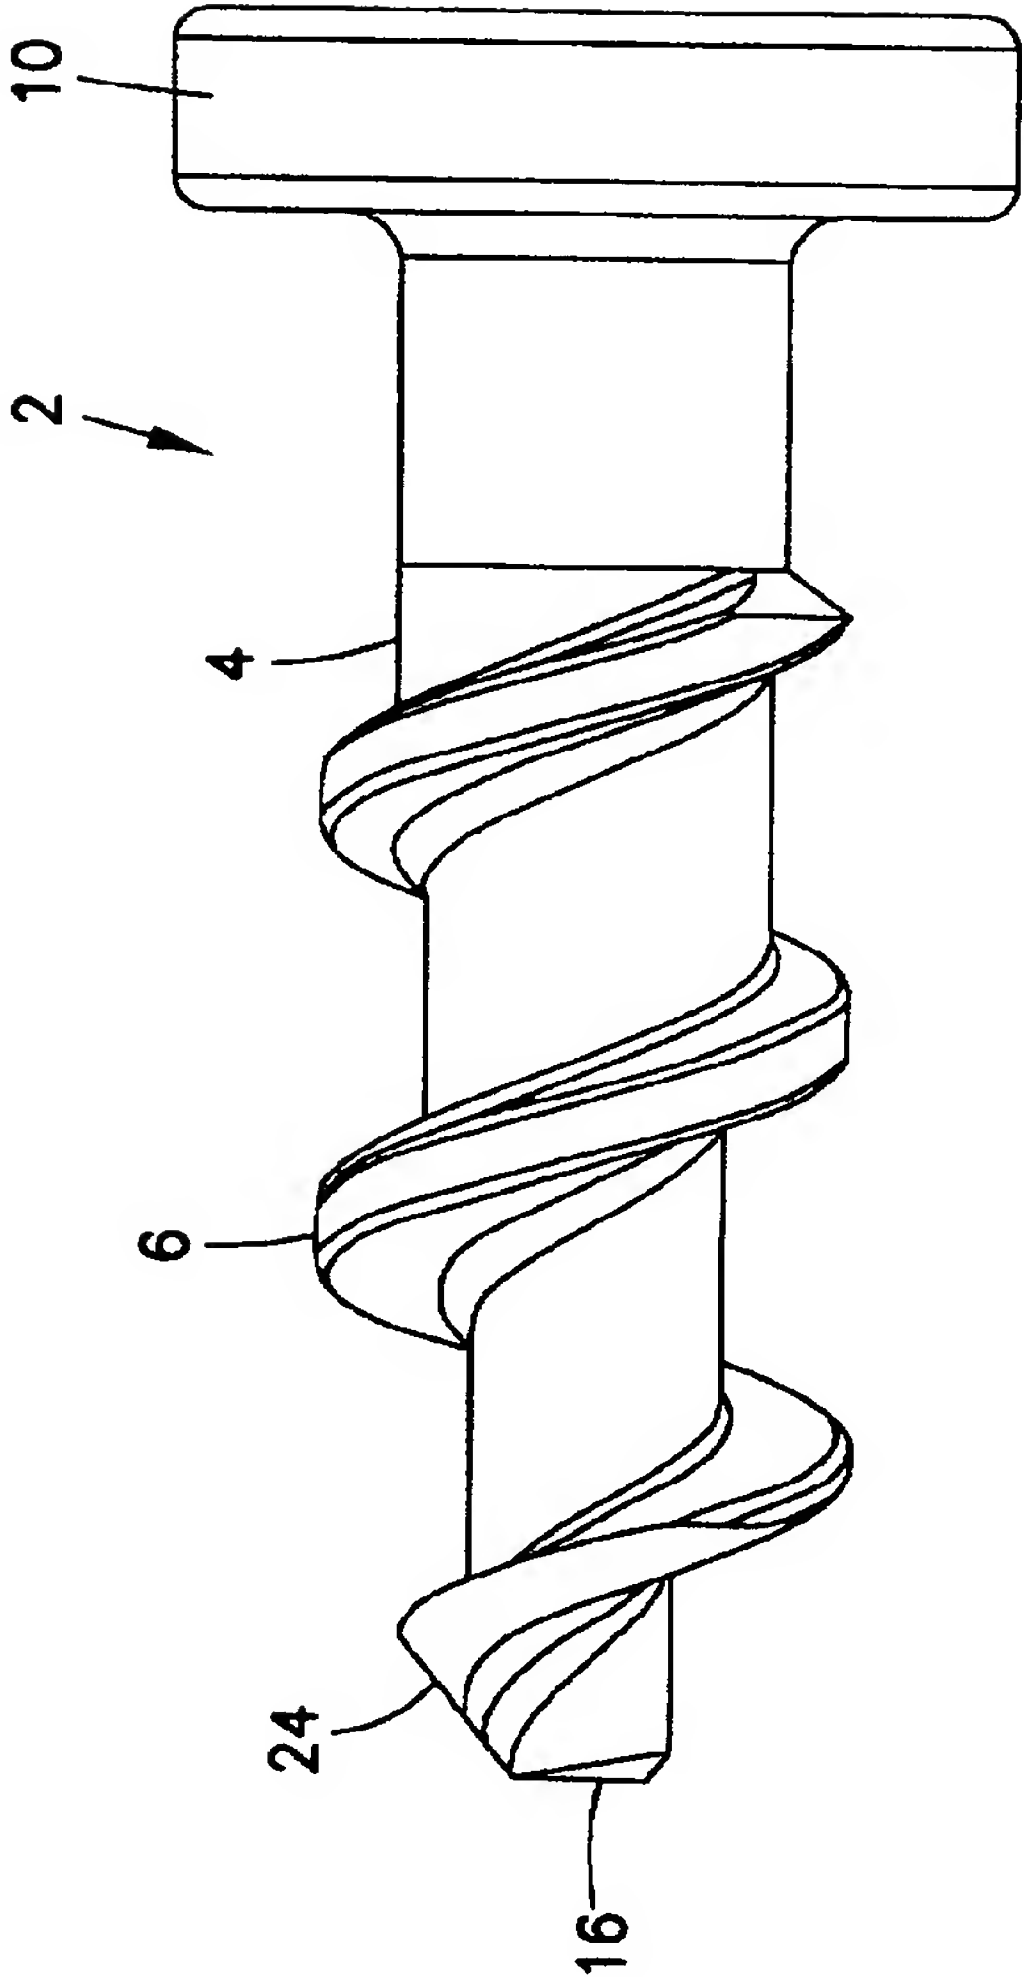


Fig. 1

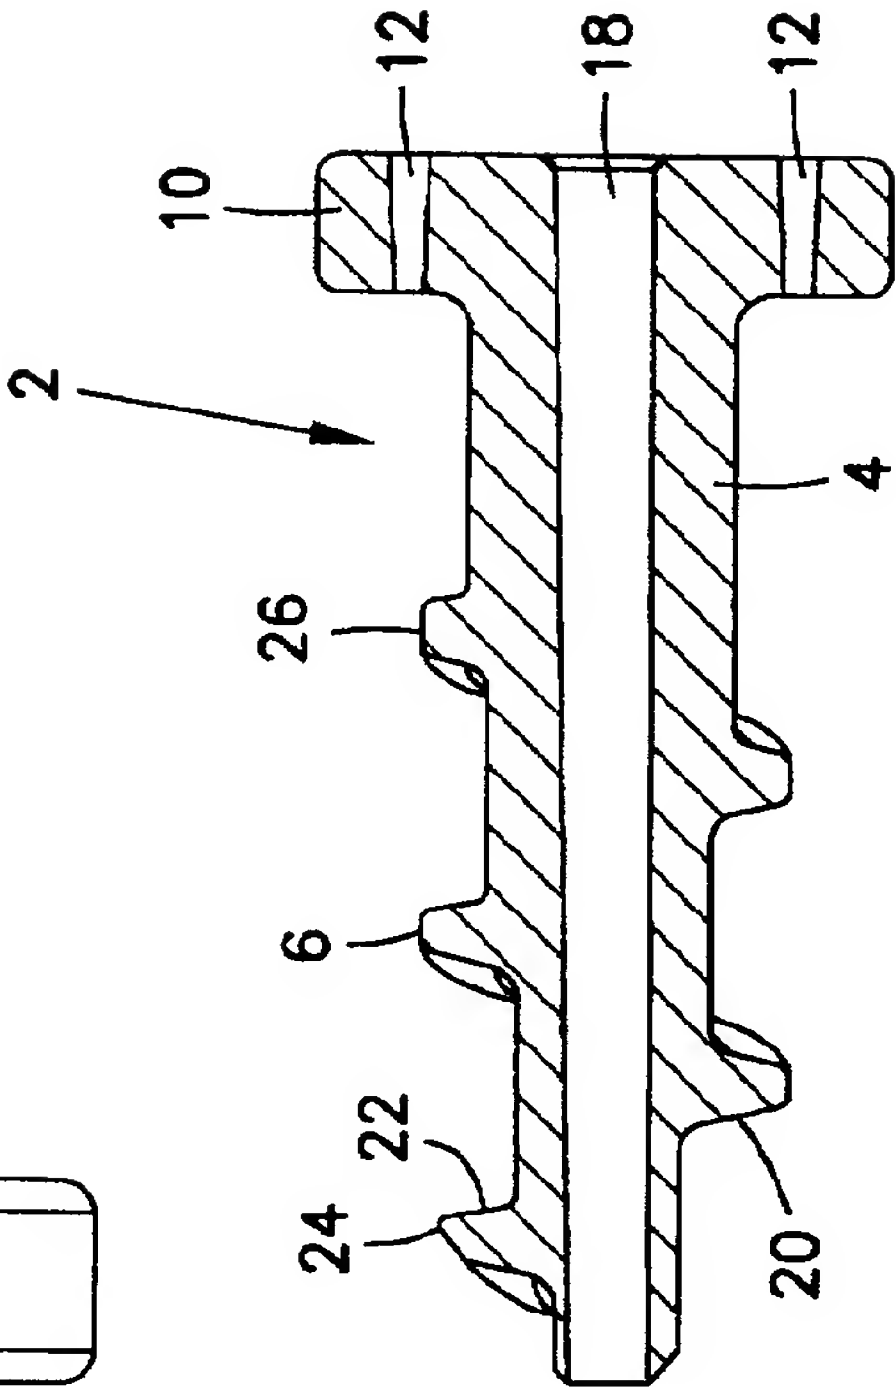


Fig. 2

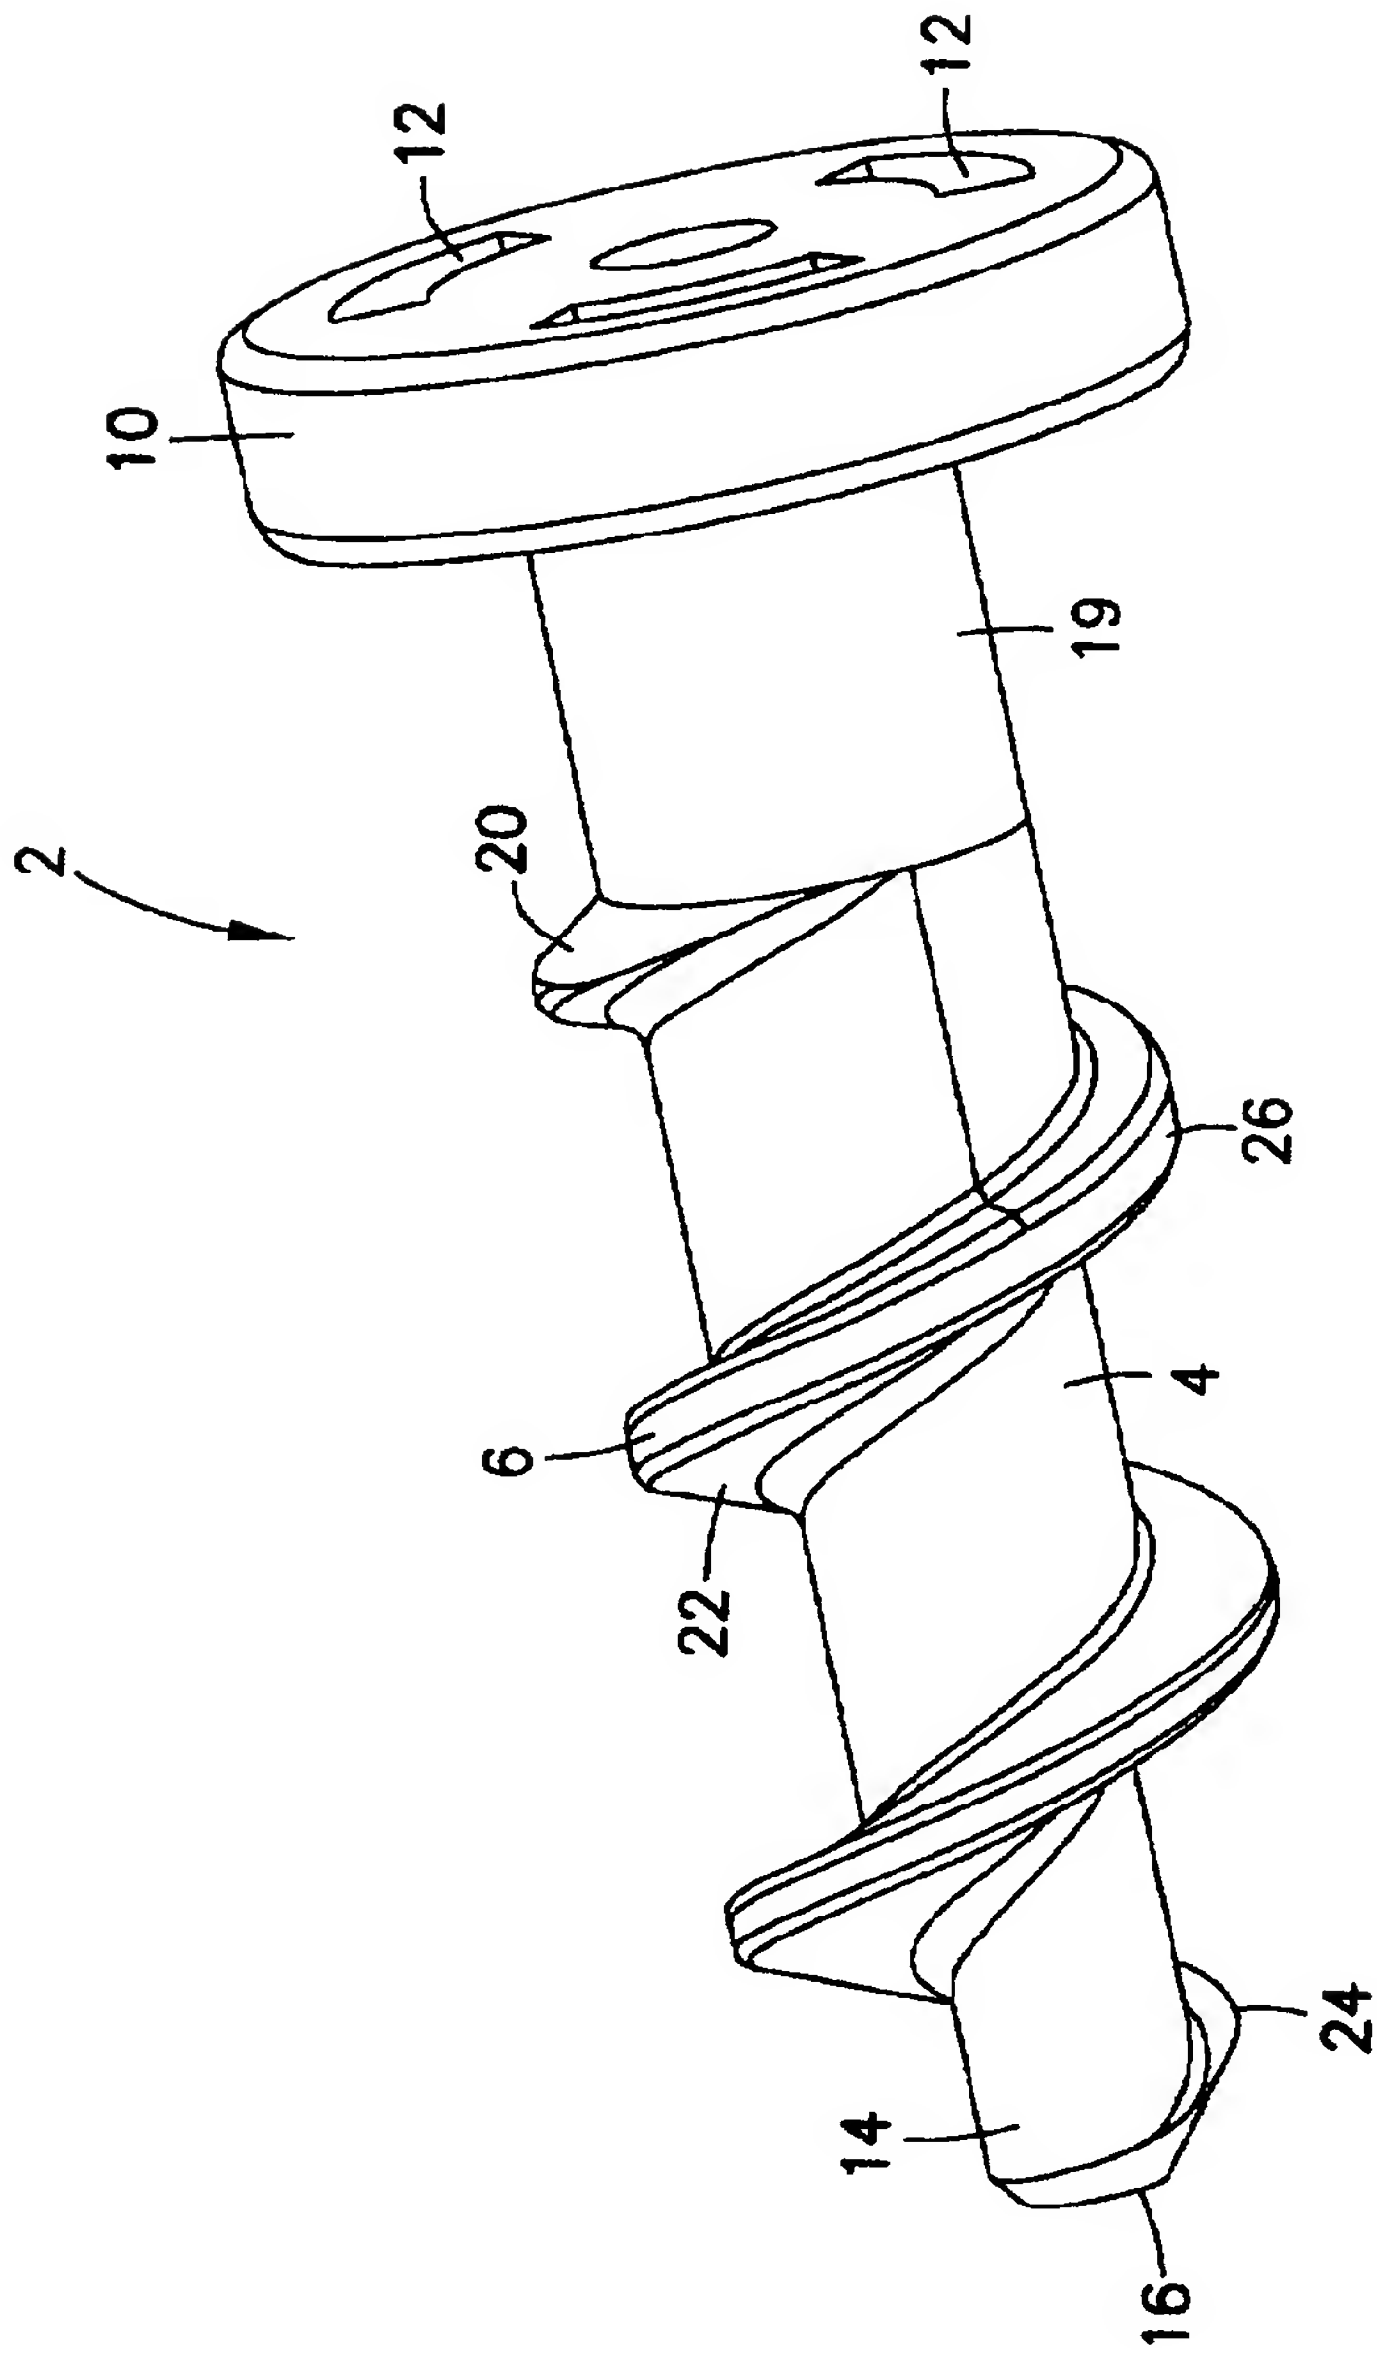


Fig. 3

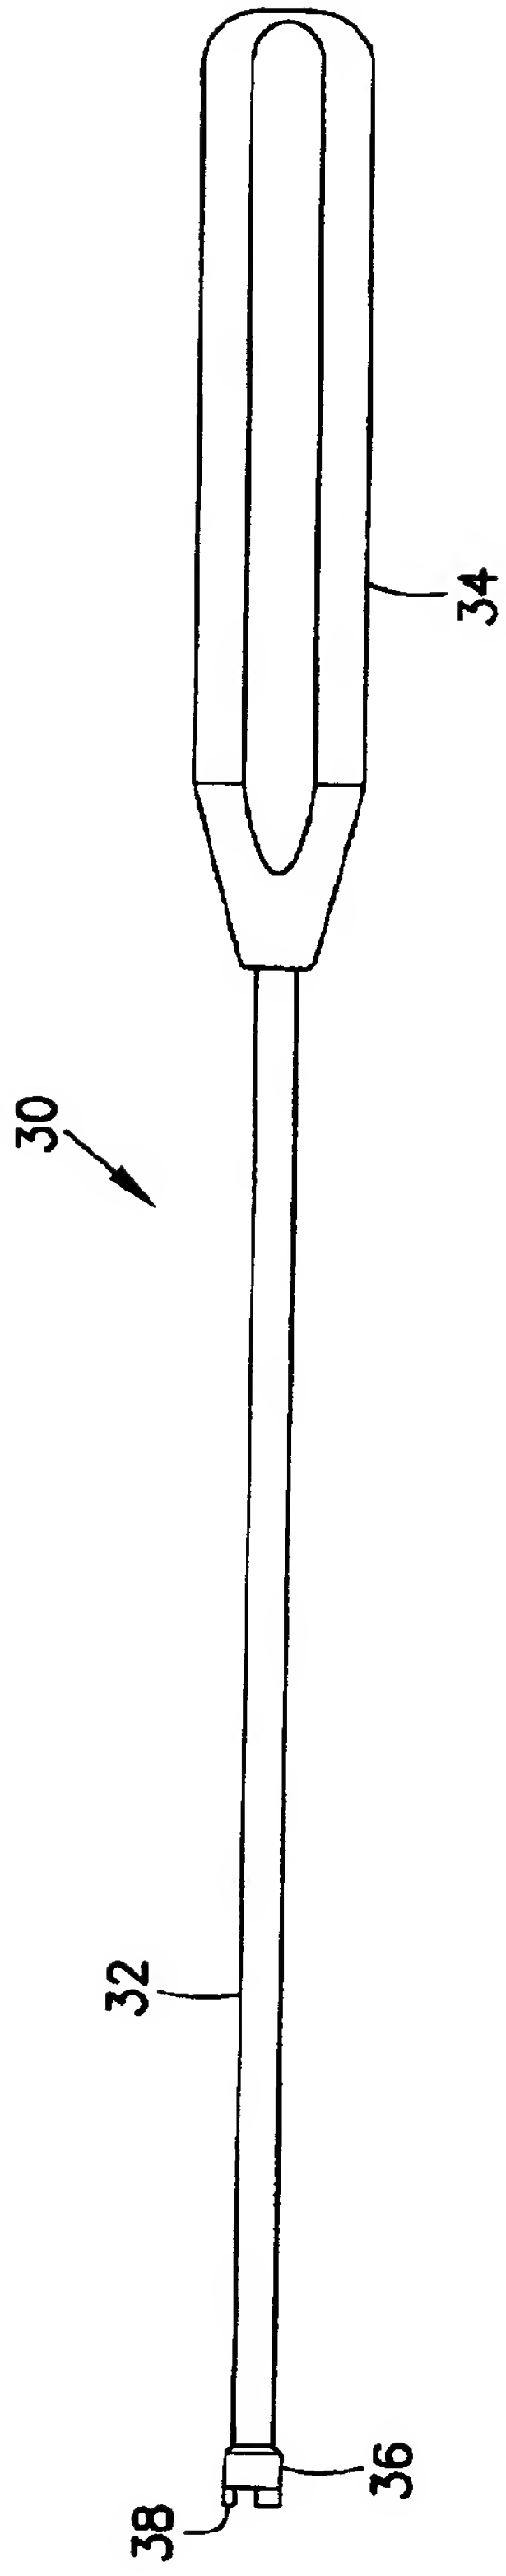


Fig. 4

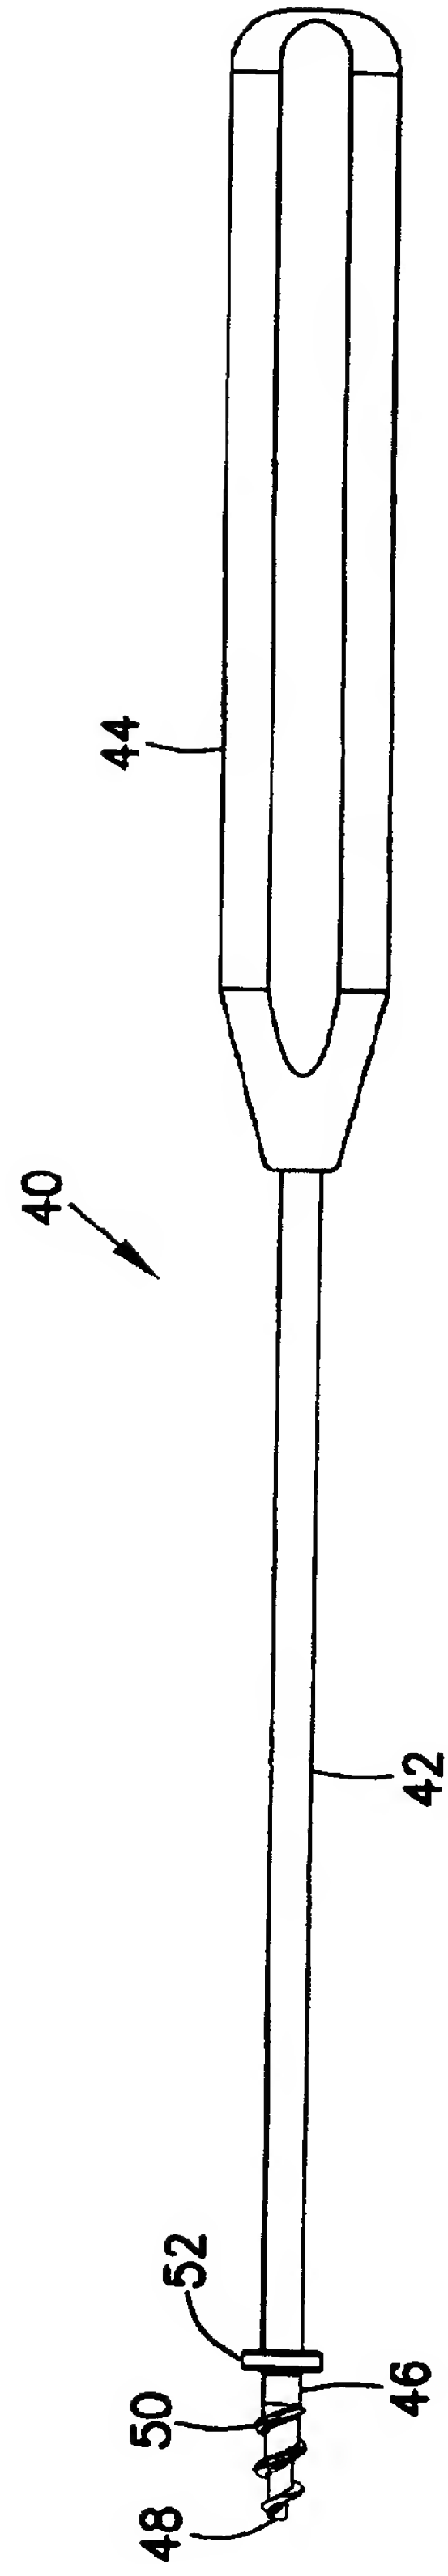


Fig. 5



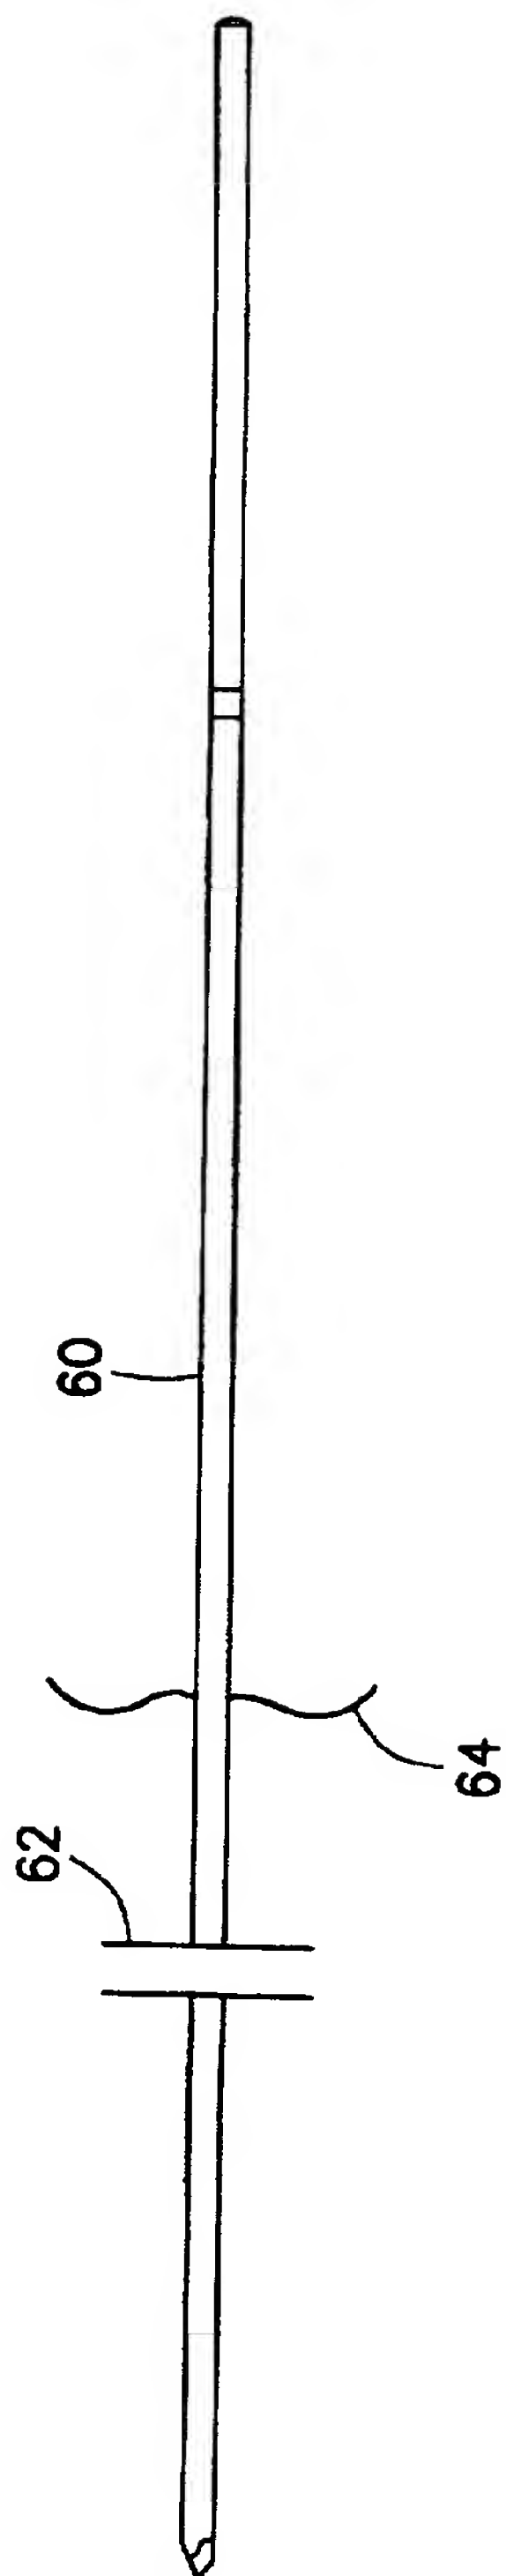


Fig. 6

70

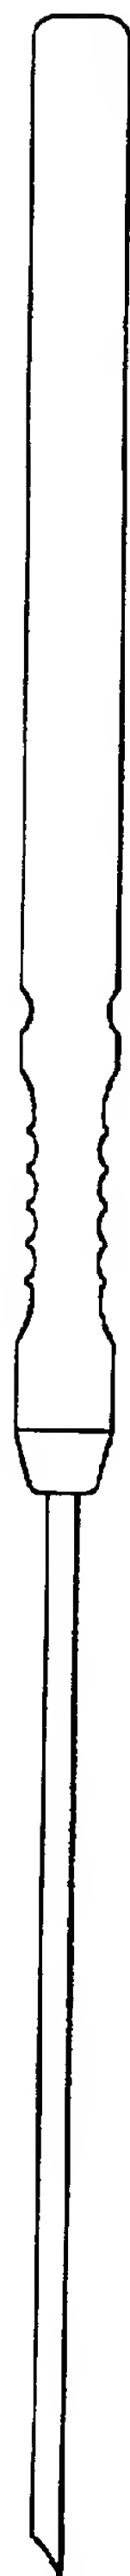


Fig. 7

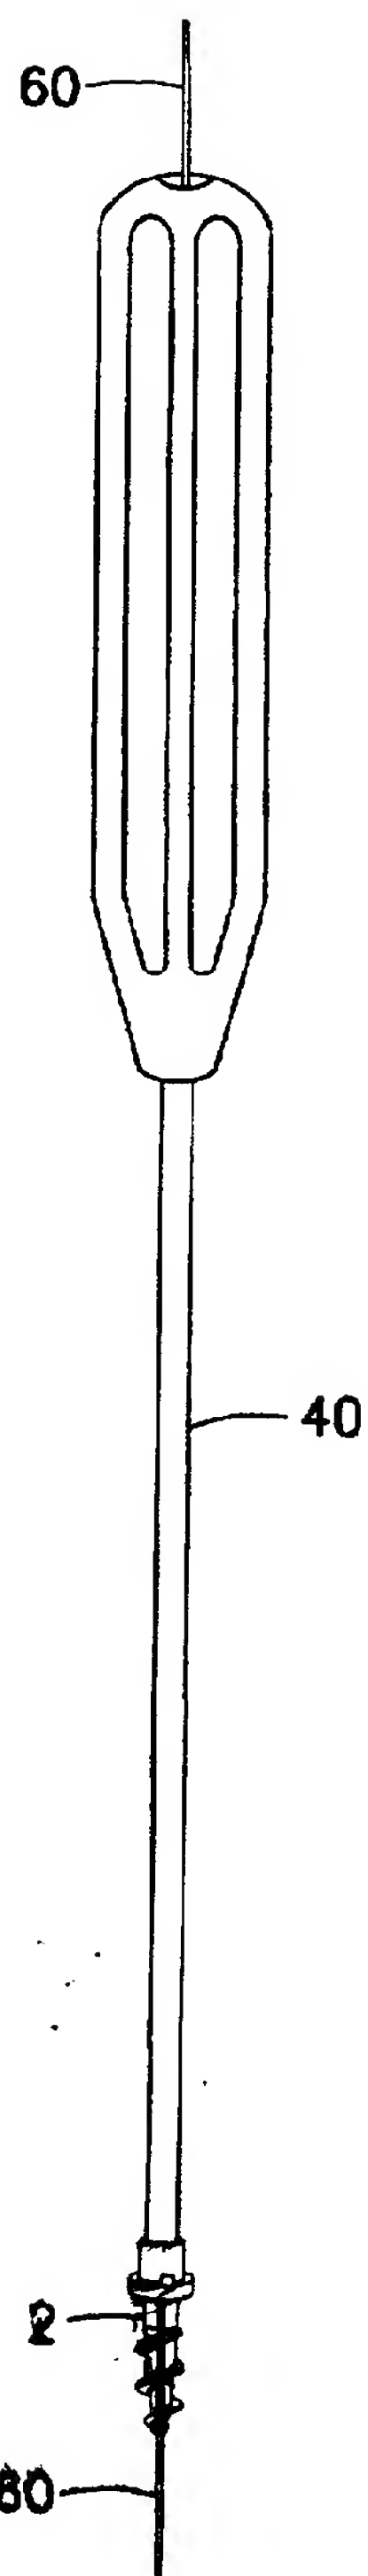


Fig. 8

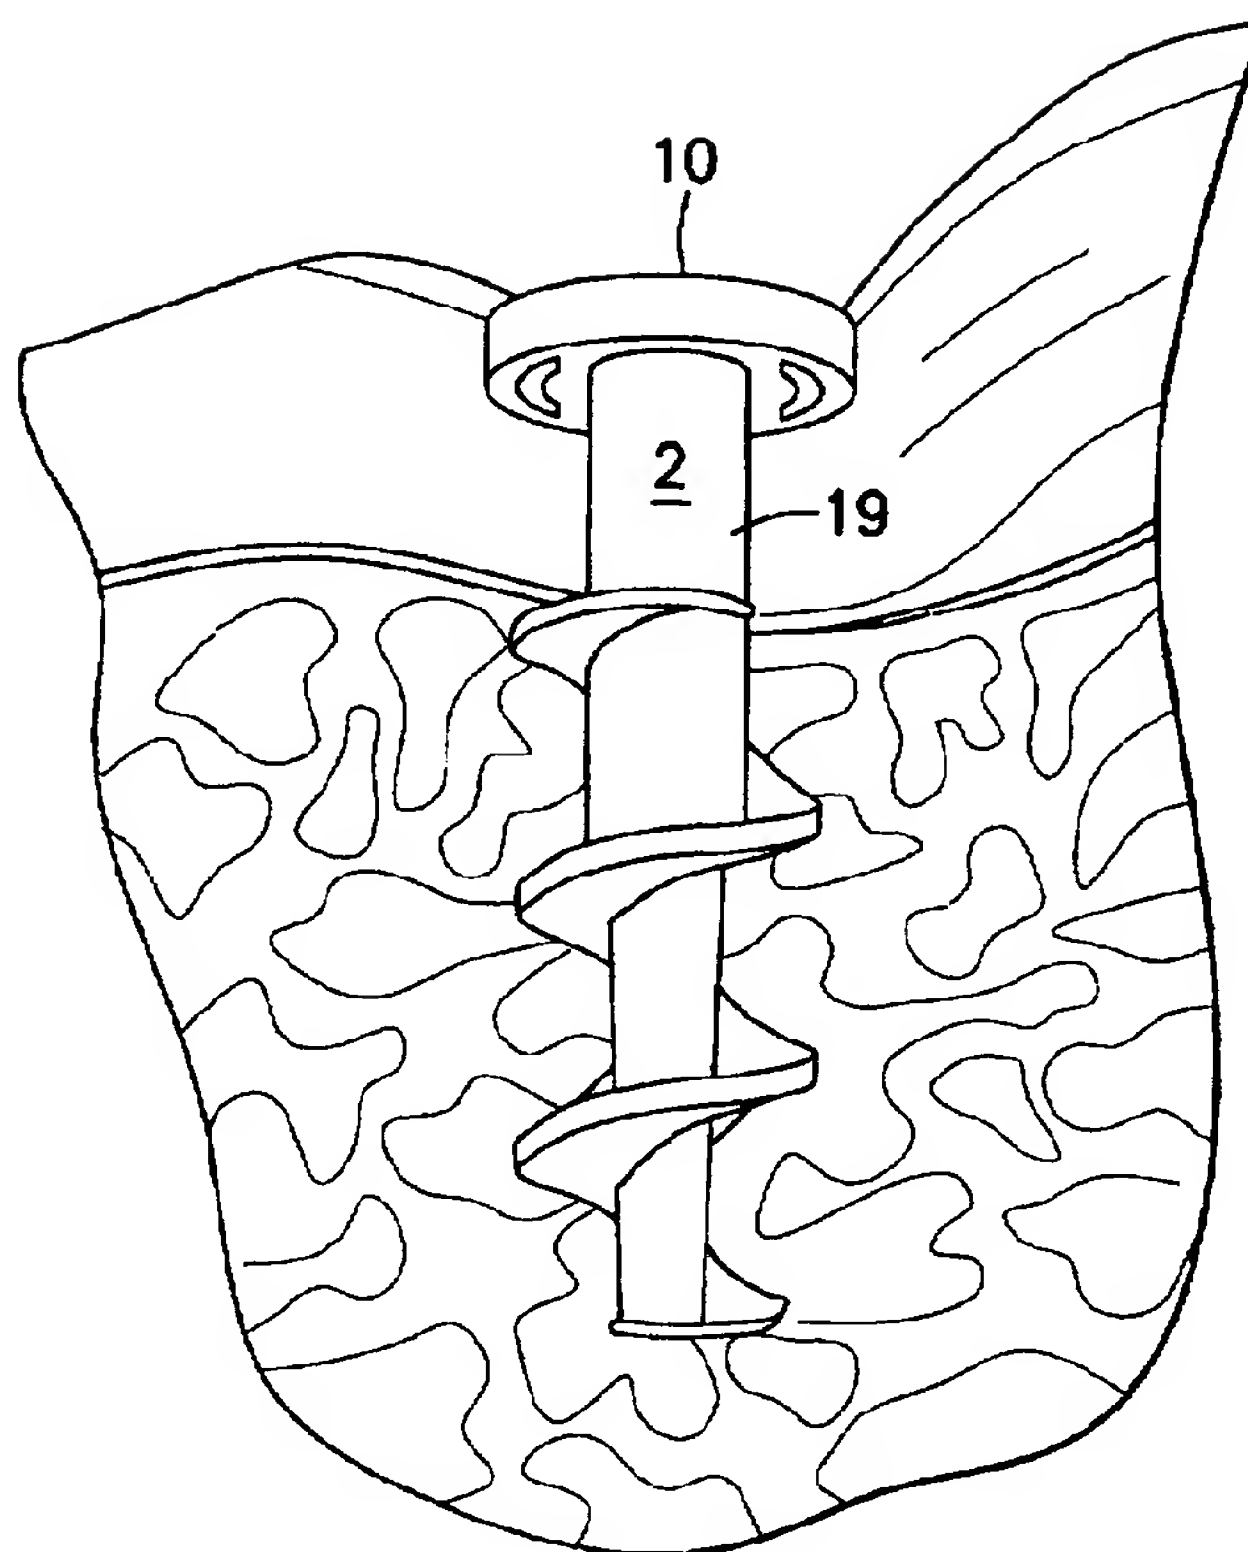


Fig. 9



European Patent  
Office

# EUROPEAN SEARCH REPORT

Application Number  
EP 00 89 0034

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int.Cl.7)
Y	EP 0 611 557 A (SMITH & NEPHEW DYONICS) 24 August 1994 (1994-08-24) * column 6, line 10 - line 16 * * column 8, line 44 - column 9, line 39; figures 2,3,3A *	1,2,6, 8-10	A61B17/04
Y	FR 2 671 717 A (ASA LABORATOIRES PROTHAID) 24 July 1992 (1992-07-24) * page 7, line 24 - line 36; figure 1 *	1,2,6, 8-10	
A	US 5 840 078 A (YERYS PAUL) 24 November 1998 (1998-11-24) * abstract; figures 3,6 *	1,2,10	
A	EP 0 686 373 A (SQUIBB BRISTOL MYERS CO) 13 December 1995 (1995-12-13) * column 4, line 23 - line 58; figures 3,4 *	1,4-7,10	
A	WO 93 21848 A (HUENE DONALD R) 11 November 1993 (1993-11-11) * abstract; figures 3-8 *	1,3,9,10	
A	EP 0 663 184 A (ETHICON INC) 19 July 1995 (1995-07-19) * abstract; figures 2,8-11 *	1,3,10	TECHNICAL FIELDS SEARCHED (Int.Cl.7)  A61B A61F
The present search report has been drawn up for all claims			
Place of search BERLIN		Date of completion of the search 16 March 2000	Examiner Hansen, S
CATEGORY OF CITED DOCUMENTS X: particularly relevant if taken alone Y: particularly relevant if combined with another document of the same category A: technological background O: non-written disclosure P: intermediate document T: theory or principle underlying the invention E: earlier patent document, but published on, or after the filing date D: document cited in the application L: document cited for other reasons &: member of the same patent family, corresponding document			

EPO FORM 1503 03.82 (Pd4C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT  
ON EUROPEAN PATENT APPLICATION NO.**

EP 00 89 0034

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.  
The members are as contained in the European Patent Office EDP file on  
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

16-03-2000

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
EP 0611557 A	24-08-1994	US 5380334 A	10-01-1995
		AT 179064 T	15-05-1999
		AU 704253 B	15-04-1999
		AU 4278097 A	12-02-1998
		AU 680214 B	24-07-1997
		AU 5516694 A	25-08-1994
		CA 2115778 A,C	18-08-1994
		DE 69417936 D	27-05-1999
		DE 69417936 T	11-11-1999
		ES 2133484 T	16-09-1999
		JP 6292686 A	21-10-1995
		US 5601558 A	11-02-1997
FR 2671717 A	24-07-1992	NONE	
US 5840078 A	24-11-1998	NONE	
EP 0686373 A	13-12-1995	US 5573548 A	12-11-1996
WO 9321848 A	11-11-1993	AT 164304 T	15-04-1998
		CA 2132298 A	11-11-1993
		DE 69317654 D	30-04-1998
		DE 69317654 T	01-10-1998
		EP 0637944 A	15-02-1995
		ES 2117131 T	01-08-1998
		JP 7509619 T	26-10-1995
EP 0663184 A	19-07-1995	AU 1011595 A	20-07-1995
		BR 9500087 A	17-10-1995
		CA 2139979 A	14-07-1995
		JP 8033640 A	06-02-1996
		US 5728116 A	17-03-1998